unicare
health

Kingfisher Bathboard
Instruction & Safety Manual

Please read this manual before operation, for maintenance instructions and safe usage

The enabling power
of applied knowledge

Kingfisher Bathboard

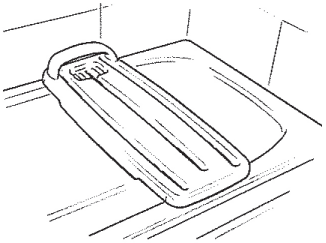

The Kingfisher Bathboard is designed to make getting in and out of the bath easier and safer. The Bathboard can also be used for showering.

Assembling the fixing brackets to the Bathboard

Four fixing brackets fir into outer slots on the underside of the Bathboard (fig.1). Hold the adjuster knob on the bracket and fit the head of the angled bolt through the 'D' shaped hole at the end of the slot (fig.2). ensuring that the bolt fits flat onto the shoulders of the slot, with the rubber buffer facing outwards. Slide the brackets towards the middle of the board.

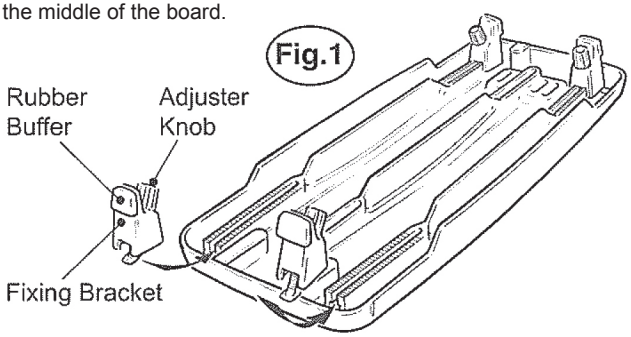



Positioning the Board in the bath

Place the Bathboard on top of the bath with the handle and/or soap dish on the wall side. Ensure that the area around is clean and ideally the board should be at the opposite end to the taps.

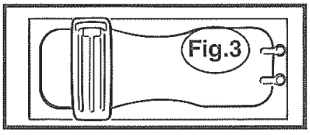

Slide the brackets our to the side of the bath. Check the position of the Bathboard and then tighten up each adjuster knob to lock the brackets in place (fig.4). Take care not to overtighten the adjuster knobs. Check that the board is secure before use. Please ensure that the fitting guide marks are over the supported area of the bath tub sides (fig.5).



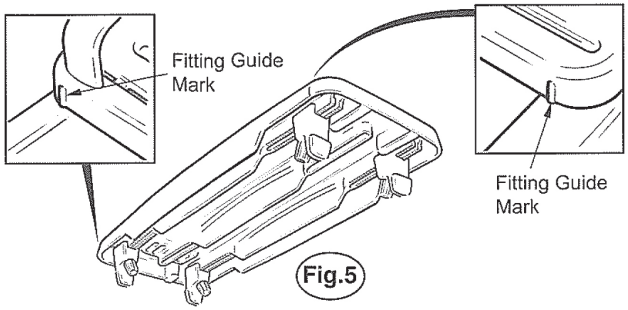

T 08 9351 7500 E info@unicarehealth.com.au W www.unicarehealth.com.au

Using the Kingfisher Bathboard
Getting in and out of the bath

Please take care getting in and out of the bath. Sit on the board with your back to the board (fig.6). Lift each leg one at a time into the bath (fig.7). Slide across to the middle of the Bathboard (fig.8). Then you may gently lower yourself down.

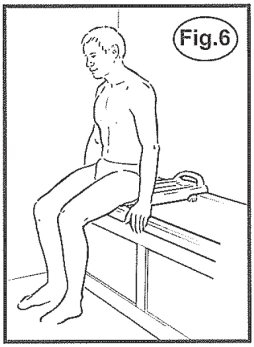

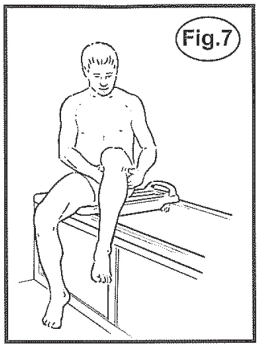

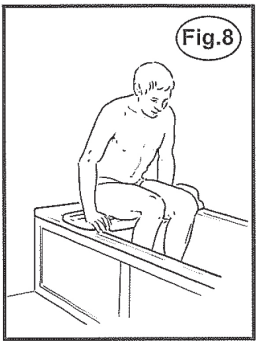

Note

For obvious safety reasons **never** sit on the edge of the Bathboard if it overlaps the bath.

It is recommended that the Bathboard be fitted where an overlap of more than 25mm exists.

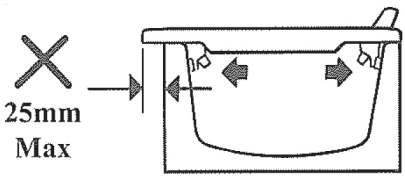

To reduce the risk of voluntary or accidental movement of the Bathboard during use, we recommend that the product is diligently checked in accordance with the attached fitting instructions every time it is fitted or re-fitted, even after a brief or temporary removal.

Cleaning

The Bathboard should be completely broken down into its component parts for cleaning as shown below. The Bathboard can be autoclaved up to 140°C and cleaned manually with any non-abrasive cleaner suitable for plastic baths. All parts should be carefully inspected for excessive wear and tear. In particular check for:

- Signs of plastic stress, white veins, cracks or surface crazing
- Excessive bending or warping
- Deformed or broken teeth on the on the underside of the body and on the feet (marked *)
- Worn out, stripped or cross-threaded screw threads

Any of these problems can lead to failure and pose a safety risk.

On re-assembly ensure that:

- The feet are properly located in the runners
- The rubber components are properly seated and do not fall out
- The handle is securely fastened in the correct orientation

The board must be supplied complete, including the instruction leaflet.

T 08 9351 7500 E info@unicarehealth.com.au W www.unicarehealth.com.au

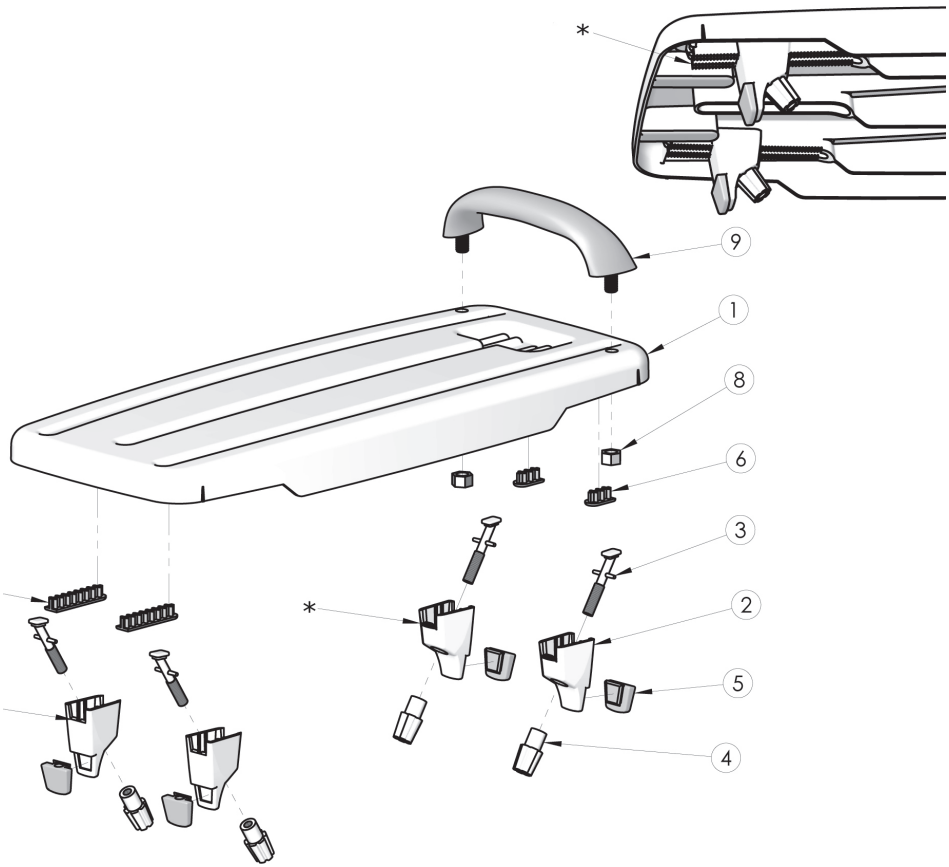

The Kingfisher Bathboard is warranted against manufacturing defects for 3 years from original purchase. The Kingsher Bathboard is designed as a single user product. The board must be completely sterilised between users to avoid cross-infection. The re-seller is responsible for ensuring the safety of the Bathboard before re-issue.

Notes

T 08 9351 7500 E info@unicarehealth.com.au W www.unicarehealth.com.au

PO Box 82 Bentley WA 6982
T 08 9351 7500 F 08 9350 5299
info@unicarehealth.com.au
www.unicarehealth.com.au

Authorised Distributor